


# Flexible Endoscopy

CW121

To complete this activity, the participant will need to access and read AORN. (2018). Flexible Endoscopes section in *Guidelines for Perioperative Practice*. (pp. 799-882). Denver, CO: AORN.

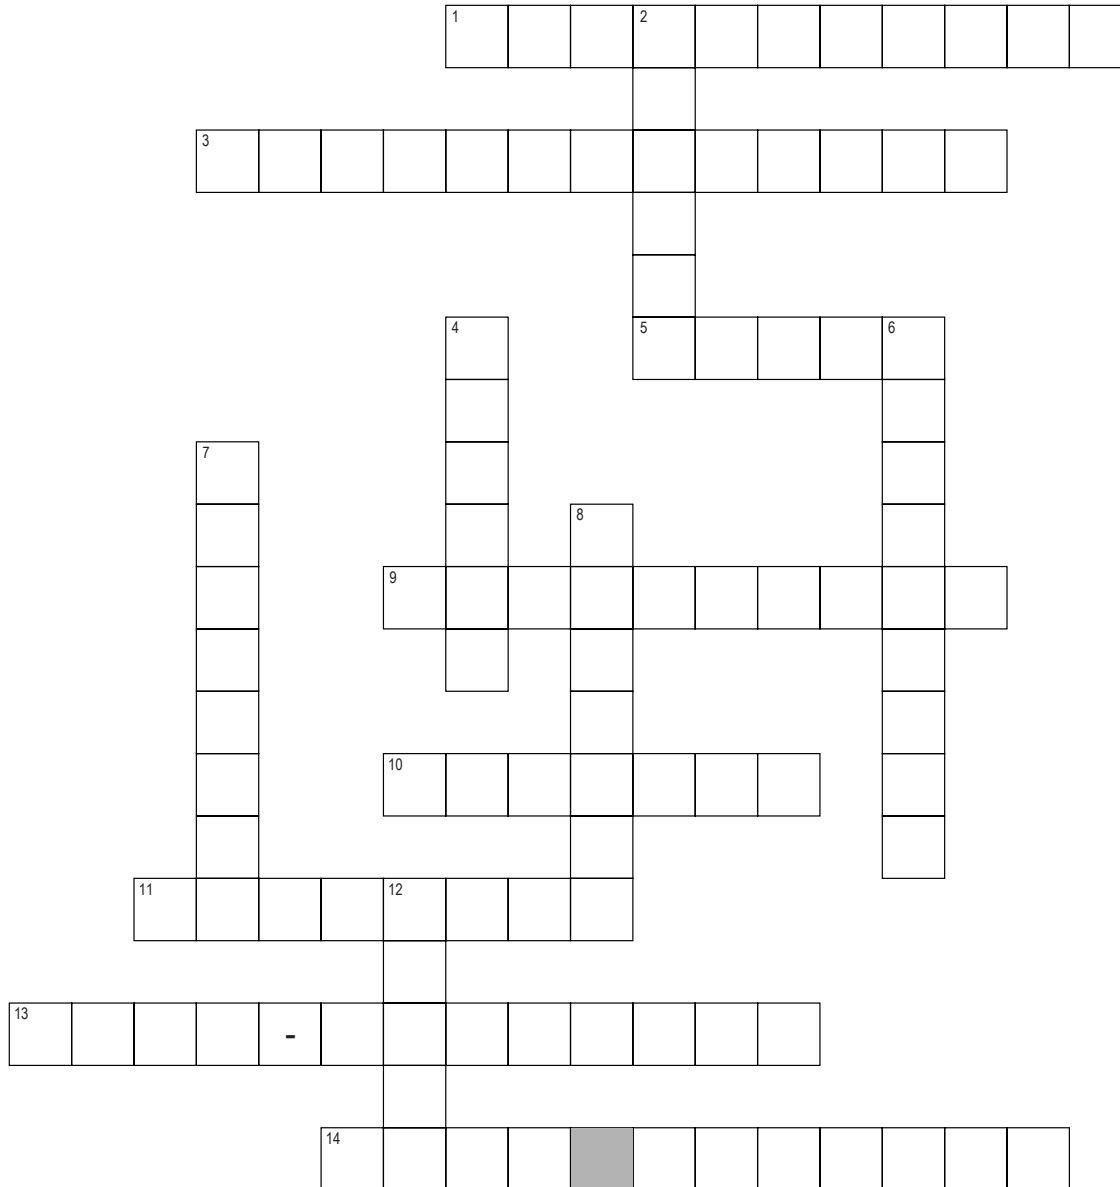

### ACROSS

1. This process should occur as soon as possible after the endoscope is removed from the patient to reduce the amount of bioburden.
3. Use of this product is not to be used in processing flexible endoscopes.
5. Storage cabinets for endoscopes should have \_\_\_\_\_ and be located a minimum of three feet from any sink.
9. The drying cabinets for endoscopes should allow for scopes to be placed \_\_\_\_\_ for drying.
10. A \_\_\_\_\_ of two decontamination sinks should be provided in the endoscopy processing room.
11. Within the decontamination room, the air pressure should be \_\_\_\_\_.
13. As a result of contact with mucous membranes, endoscopes are considered \_\_\_\_\_ items according to Spaulding classification system. (hyphenated word)
14. This process should occur before the endoscope is manually cleaned and placed into the cleaning solution. (2 words)

### DOWN

2. Transporting of contaminated endoscopes to decontamination area requires a \_\_\_\_\_ container.
4. Flexible endoscopes should be stored with \_\_\_\_\_ open and removable parts detached.
6. The classification system that determines high level disinfection for endoscopes.
7. Within the clean workroom, the air pressure should be \_\_\_\_\_.
8. \_\_\_\_\_ water should be used when performing the mechanical processing of flexible endoscopes.
12. The minimum number of functional areas for an endoscopy site.

\* Content reviewed by the CCI Nursing Education Department for alignment with clinical practice standards. CCI does not require, recommend, or endorse specific training programs in specialized practice areas for any of its exams. This is an example of a future points activity for recertification in collaboration with CCI.

