


# Cleaning and Care of Surgical Instruments

CW124

To complete this activity, the participant will need to access and read AORN. (2018). *Cleaning and Care of Surgical Instruments. Guidelines for Perioperative Practice.* (pp. 907-942). Denver, CO: AORN.

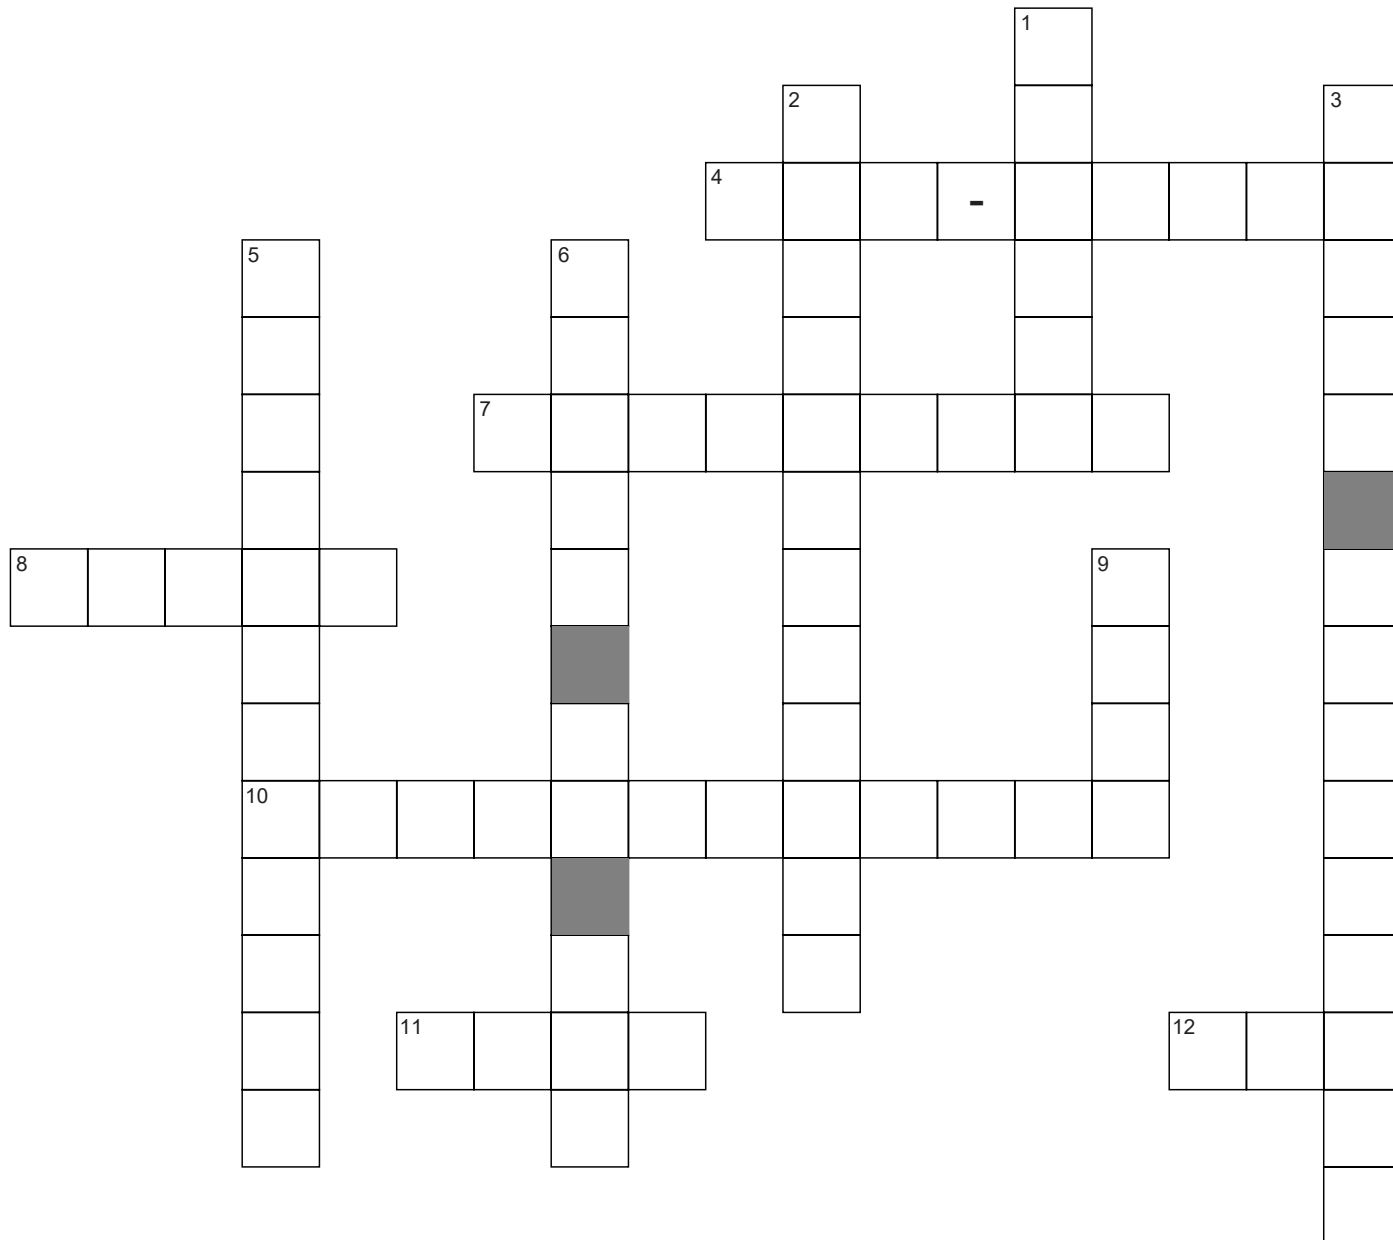

## ACROSS

4. According to the Spaulding classification system, laryngoscope handles require \_\_\_\_\_ disinfection.
7. Liquids to soak instruments must be \_\_\_\_\_ before transport of the contaminated items.
8. Instruments should be kept \_\_\_\_\_ until they are cleaned to prevent the build-up of biofilm.
10. Provides the instructions for use regarding instruments and medical devices.
11. A complication resulting from inadequate cleaning of eye instruments. (abbreviation)
12. This organization clears all instruments and devices for use in the OR. (abbreviation)

## DOWN

1. The use of \_\_\_\_\_ is not recommended when cleaning instruments due to the potential for corrosion.
2. Upon receipt at the facility, loaner instruments should be considered \_\_\_\_\_ and delivered to sterile processing.
3. Gowns used as PPE in the decontamination area must be \_\_\_\_\_. (2 words)
5. To ensure contact with the cleaning solution, instruments with multiple parts should be \_\_\_\_\_.
6. Decontamination of instruments should begin at the \_\_\_\_\_. (3 words)
9. The recommended distance between the sterilization area and instrument washing area is \_\_\_\_\_ feet.

\* Content reviewed by the CCI Nursing Education Department for alignment with clinical practice standards. CCI does not require, recommend, or endorse specific training programs in specialized practice areas for any of its exams. This is an example of a future points activity for recertification in collaboration with CCI.

