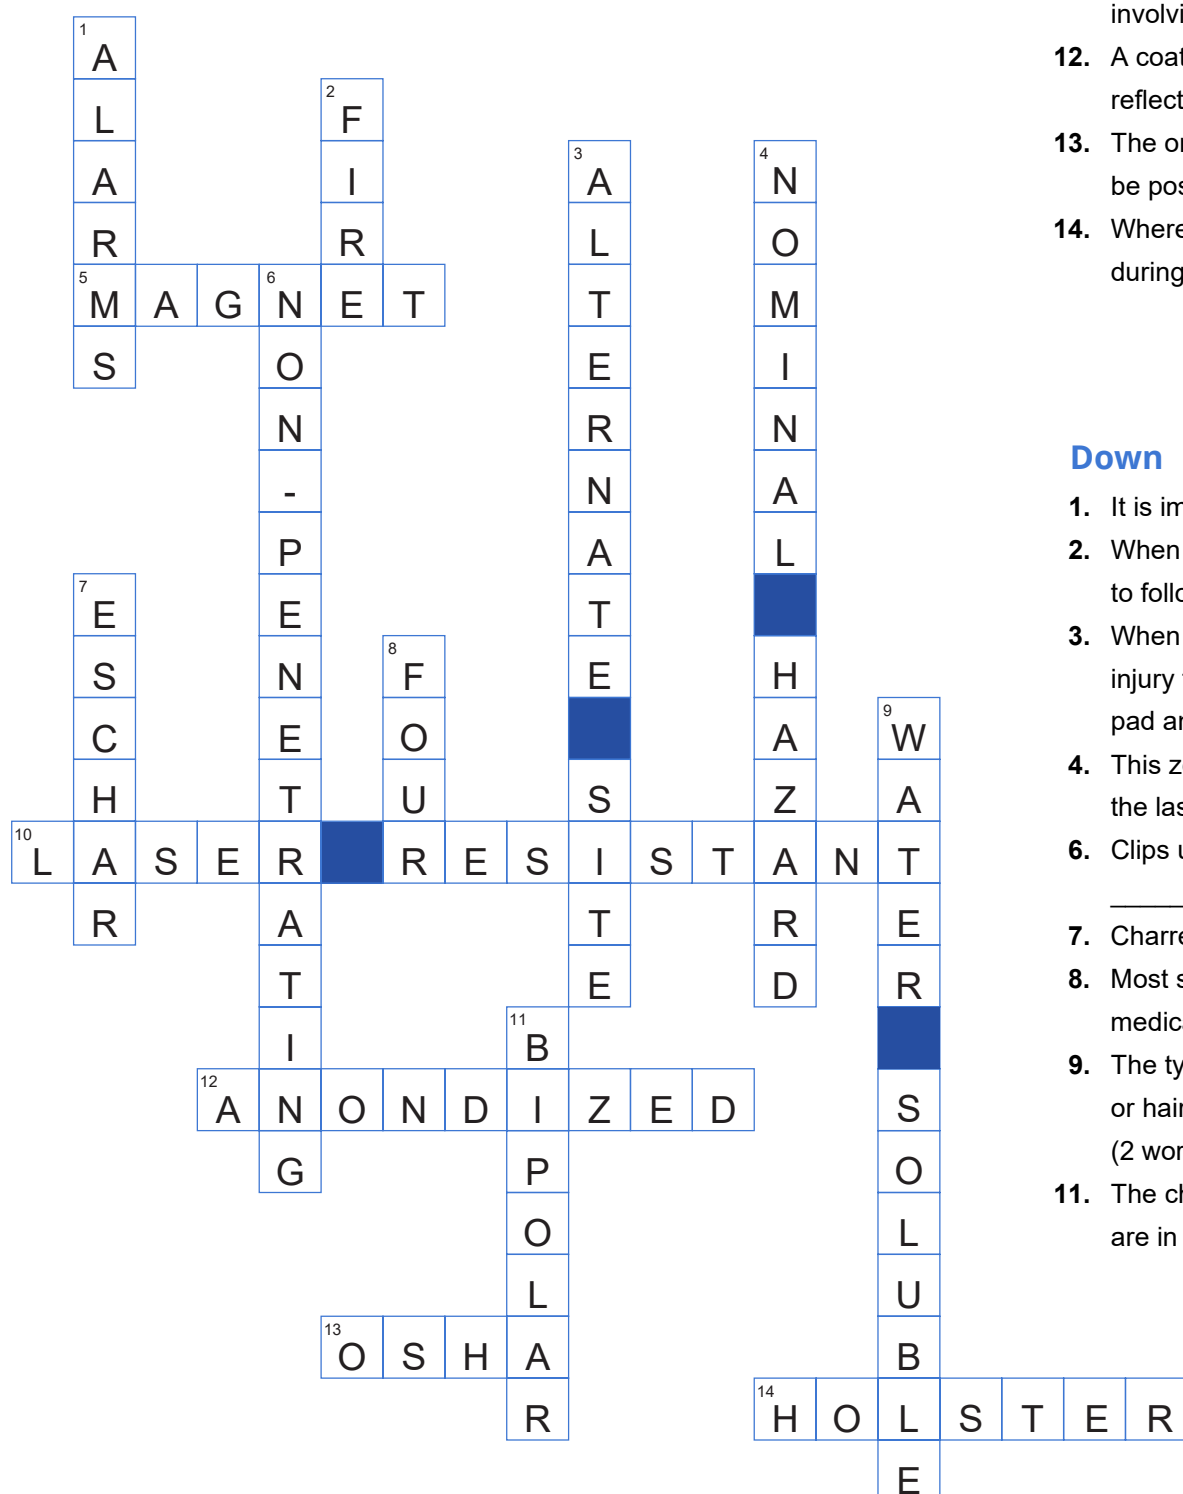


Energy Generating Devices

CW139 ANSWER KEY

To complete this activity, the participant will need to access and read the Energy Generating Devices section within the *2020 AORN Guidelines for Perioperative Practice*. AORN. (2020).

**Across**

5. It is important to have this piece of equipment available if a surgical patient has a pacemaker.
10. Endotracheal tubes must be _____ in laser cases involving the airway. (2 words)
12. A coating applied to surgical instruments to decrease reflectivity.
13. The organization that requires a laser warning sign to be posted in areas of laser use.
14. Where the cautery pencil is placed when not in use during a procedure.

Down

1. It is important that _____ are audible at all times.
2. When using energy generating devices, it is important to follow _____ precautions.
3. When cautery is used there is a risk for an _____ injury to occur if there is metal between the dispersive pad and the ESU pencil. (2 words)
4. This zone requires all staff to wear eye protection when the laser is in use. (2 words)
6. Clips used to secure cords to the drapes should be _____ and not metal. (Hyphenated)
7. Charred tissue residue.
8. Most surgical lasers are considered class _____ medical devices.
9. The type of lubricant that should be used near the eyes or hair when using any energy generating device. (2 words)
11. The choice of cautery when neuromonitoring devices are in use.